



TN11171: Installing the VTX423 Sensor

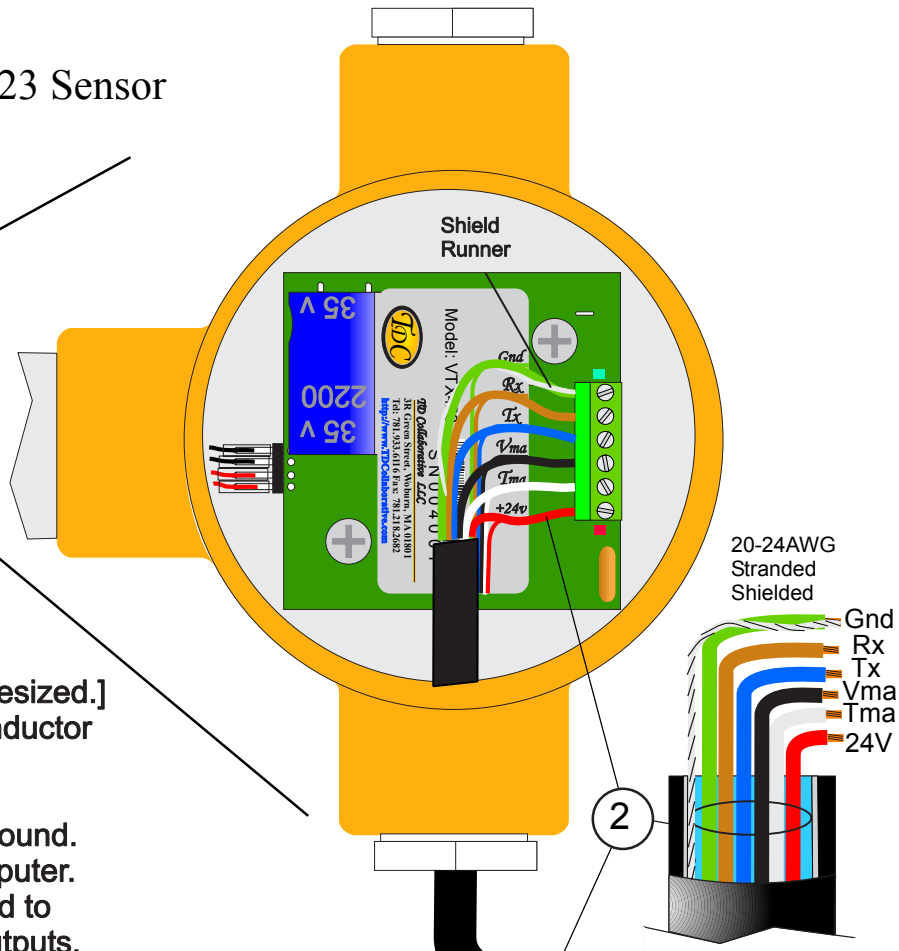

1. Mount sensor in 1" pipe Tee. [Or as resized.]
2. Connect sensor to Display with 6 conductor 20-24AWG shielded stranded cable. Ground shield at both ends.
3. Connect display to a reliable earth ground.
4. [Optional] Connect serial port to computer.
5. [Optional] Connect up to 250ohm load to 4-20ma viscosity and temperature outputs.
6. Connect ac adaptor to 24Vdc power jack.
7. Plug adaptor into universal mains power.

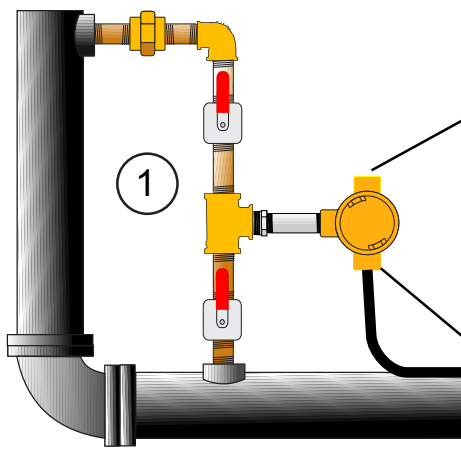